

FIG. 1

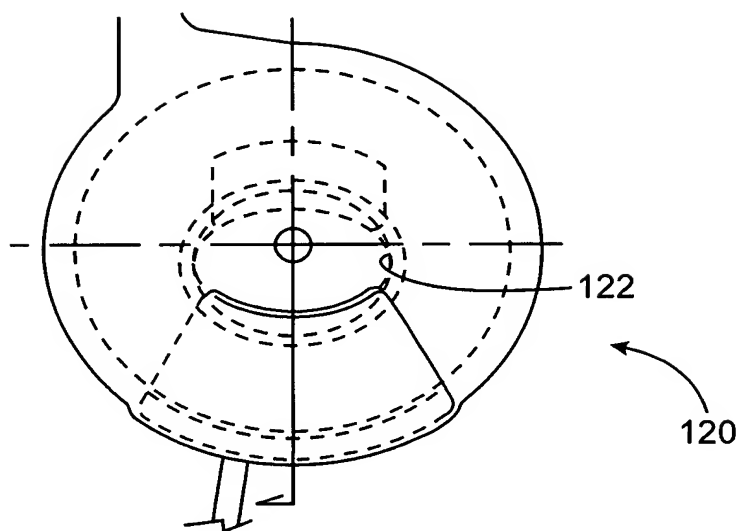


FIG. 2

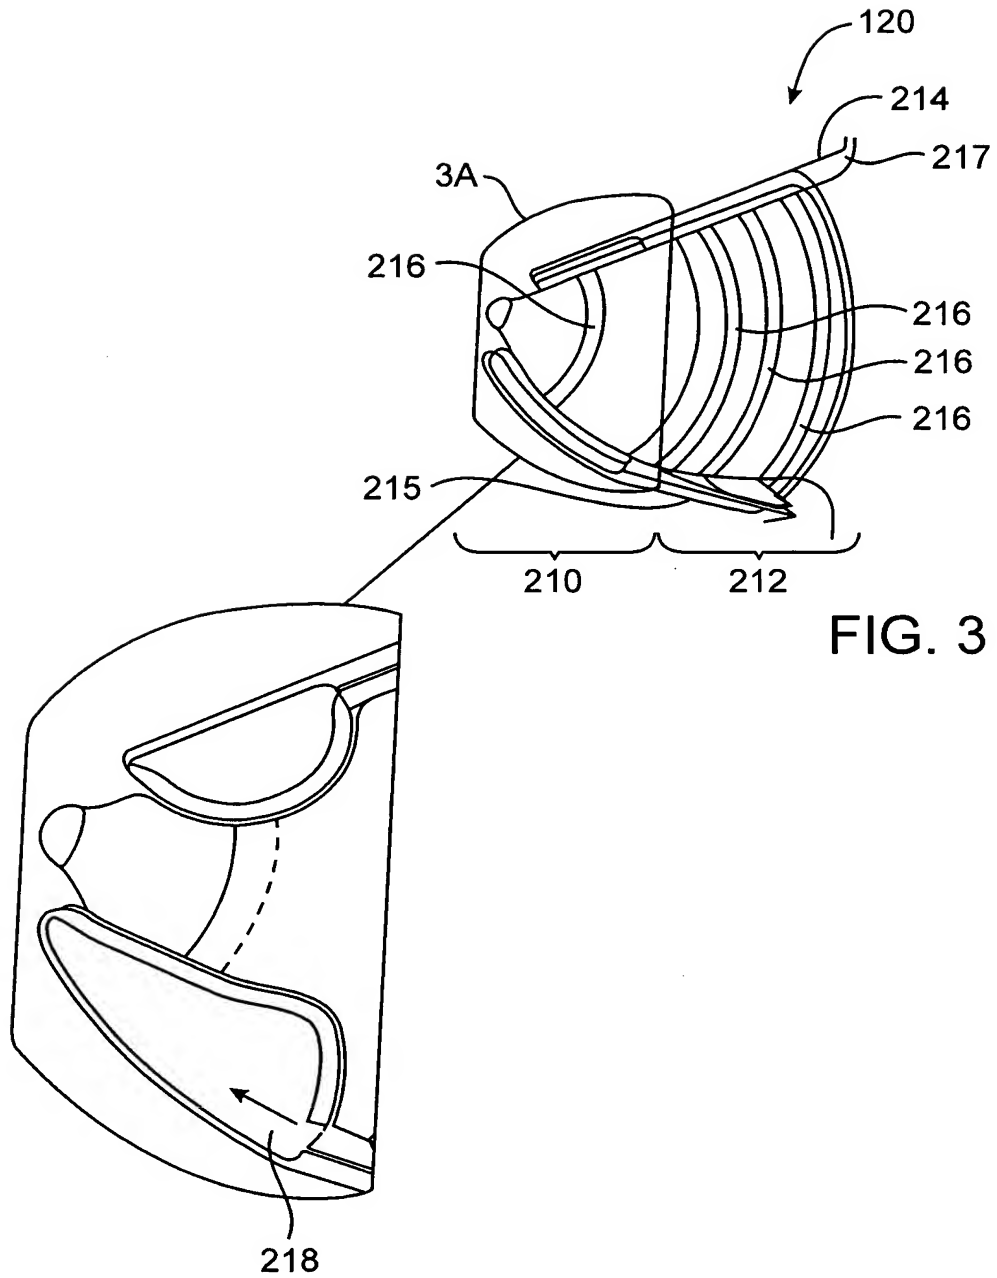


FIG. 3

FIG. 3A

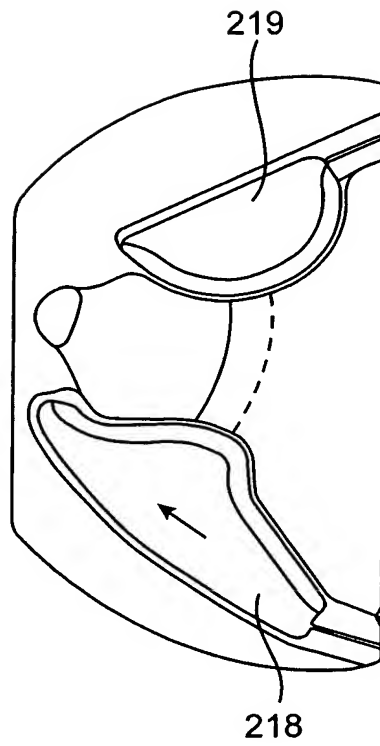


FIG. 3B

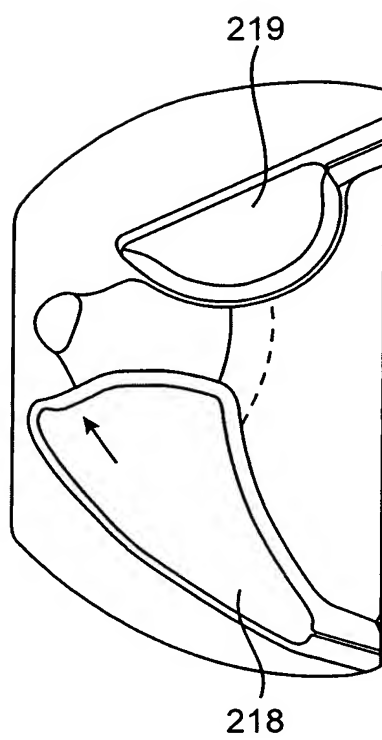


FIG. 3C

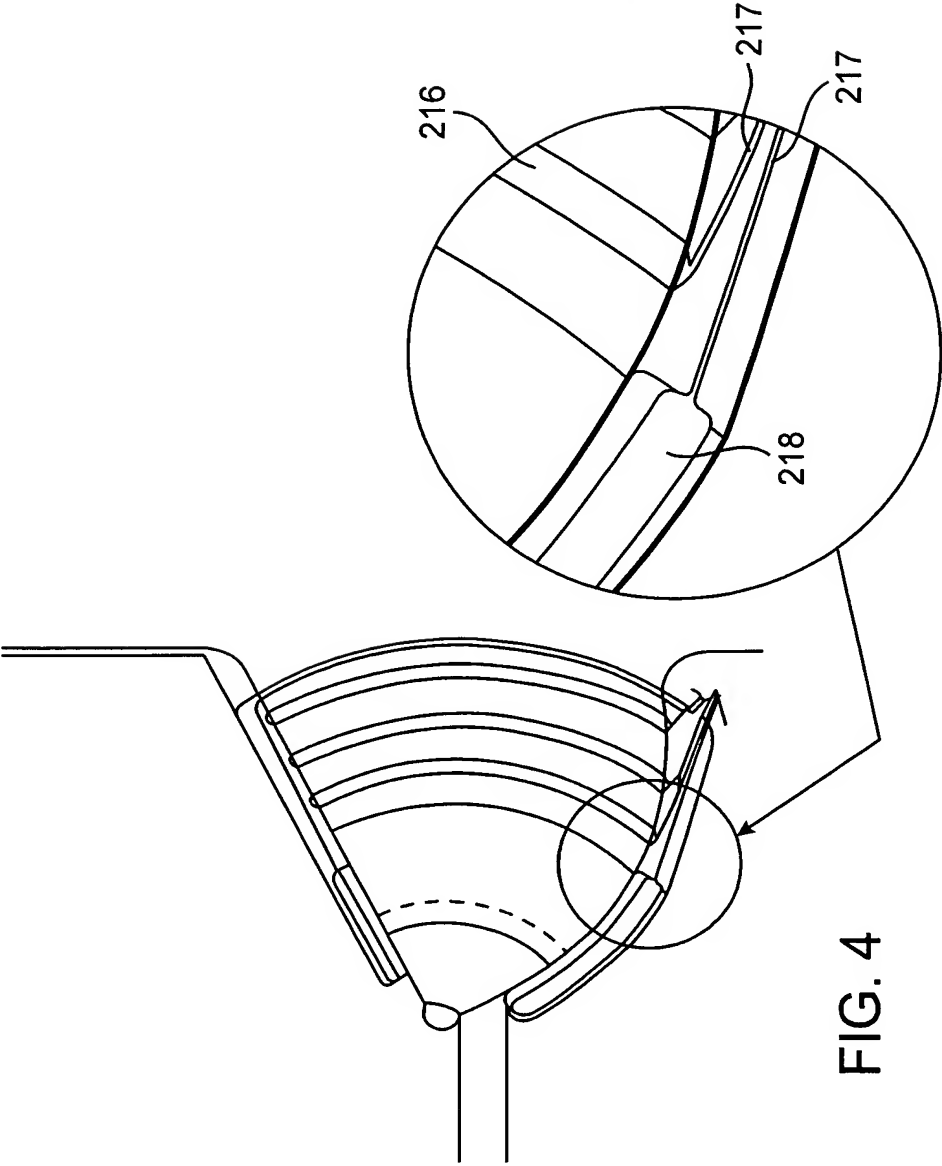


FIG. 4

FIG. 4A

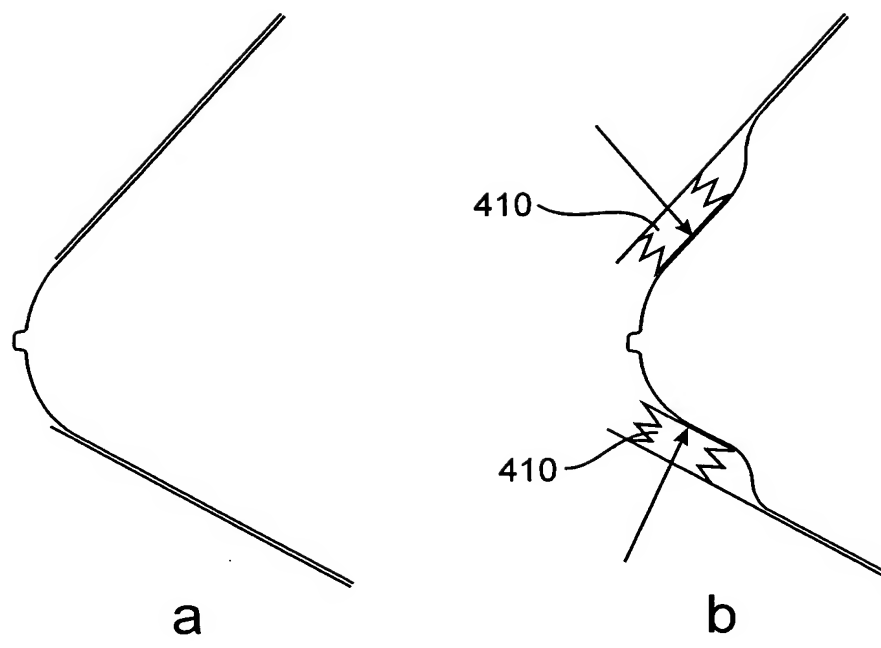


FIG. 5

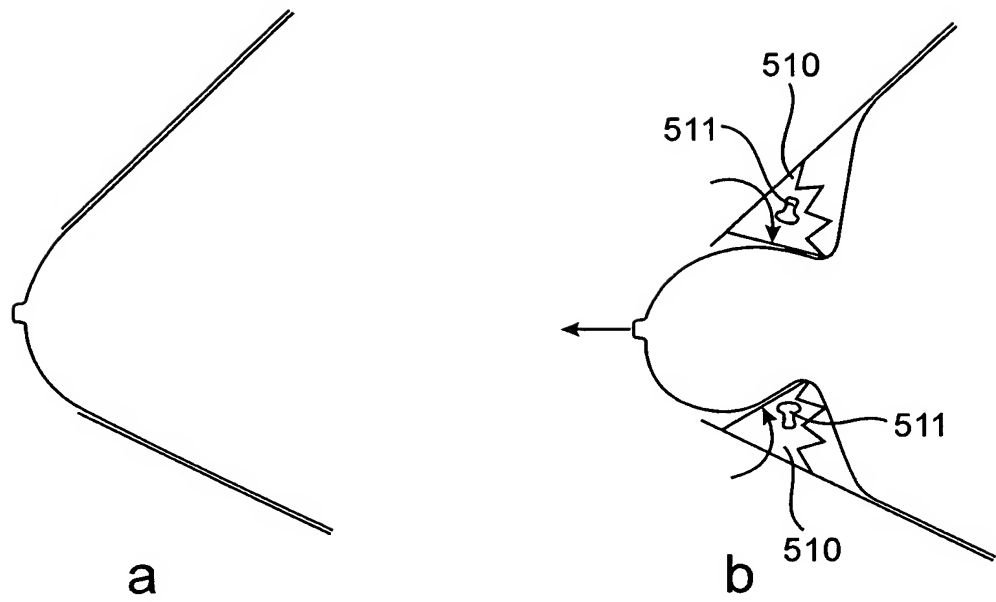


FIG. 6



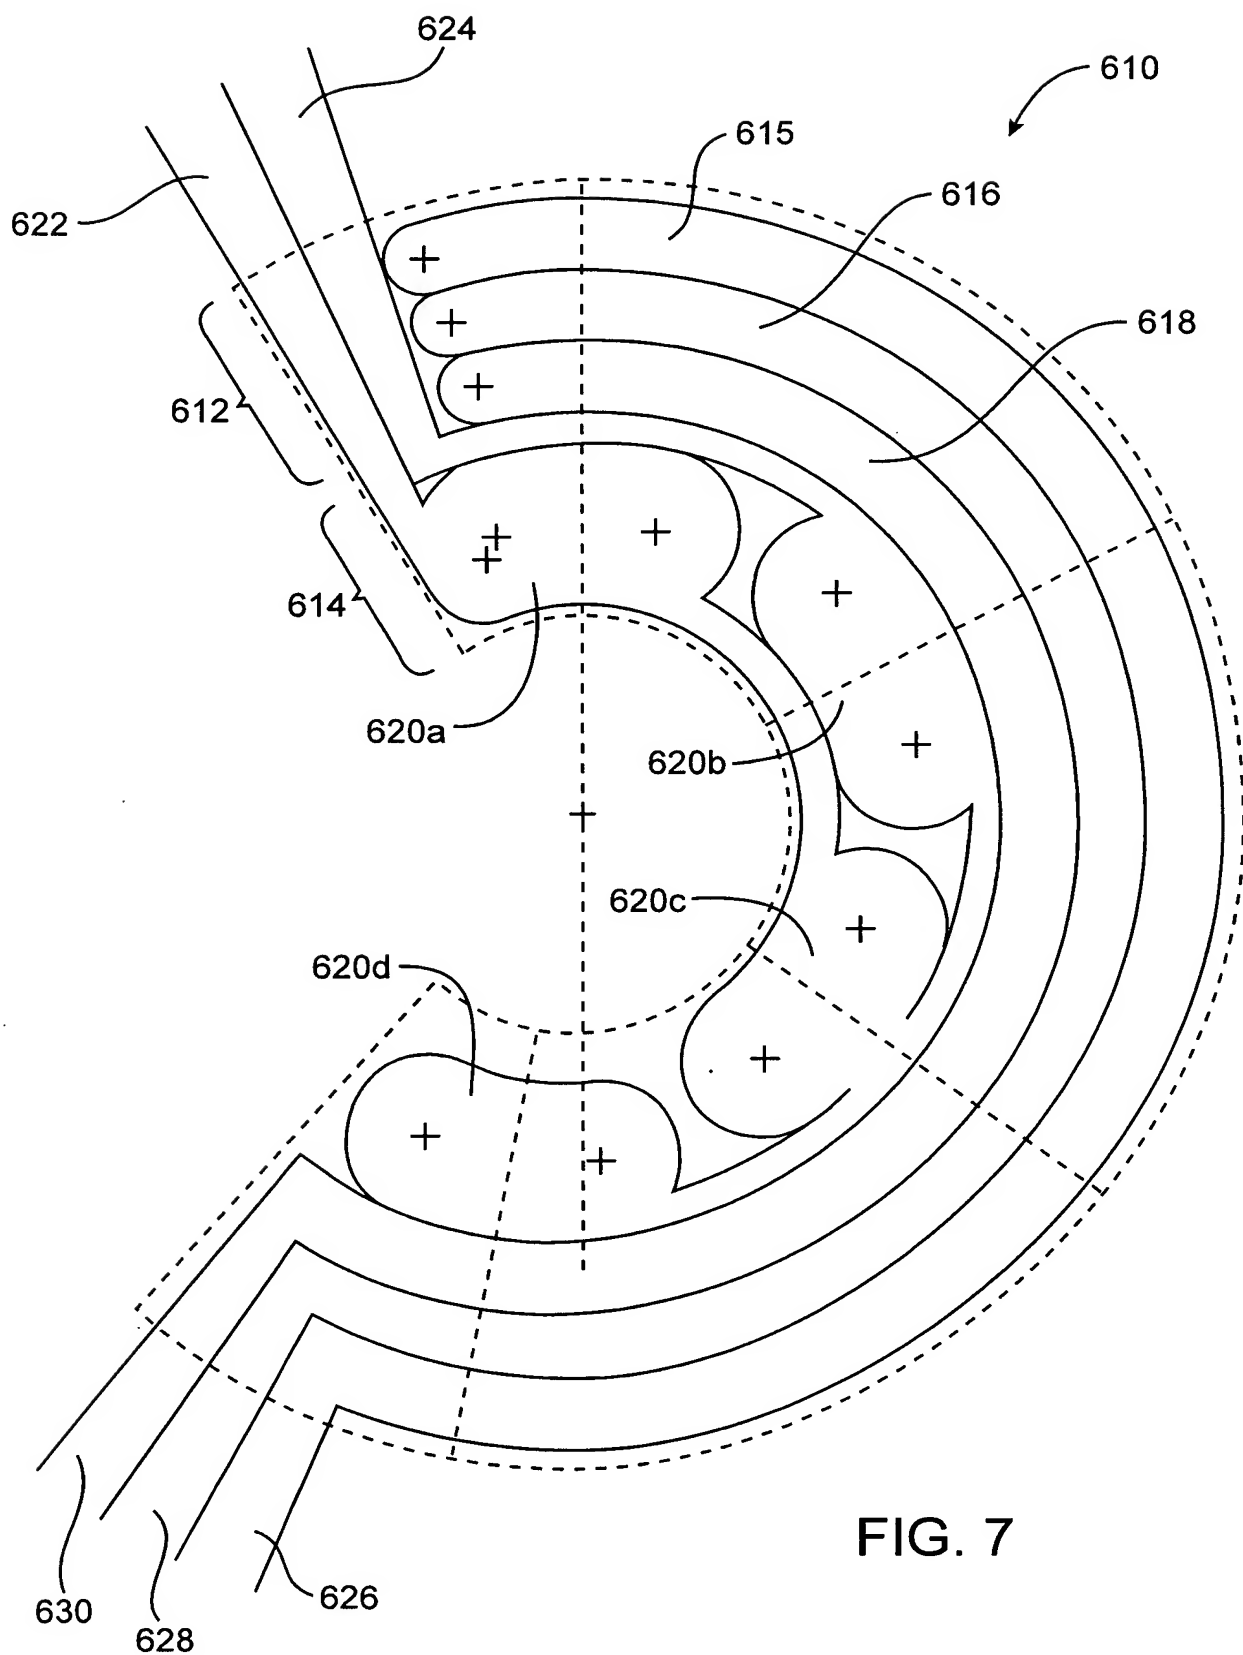


FIG. 7

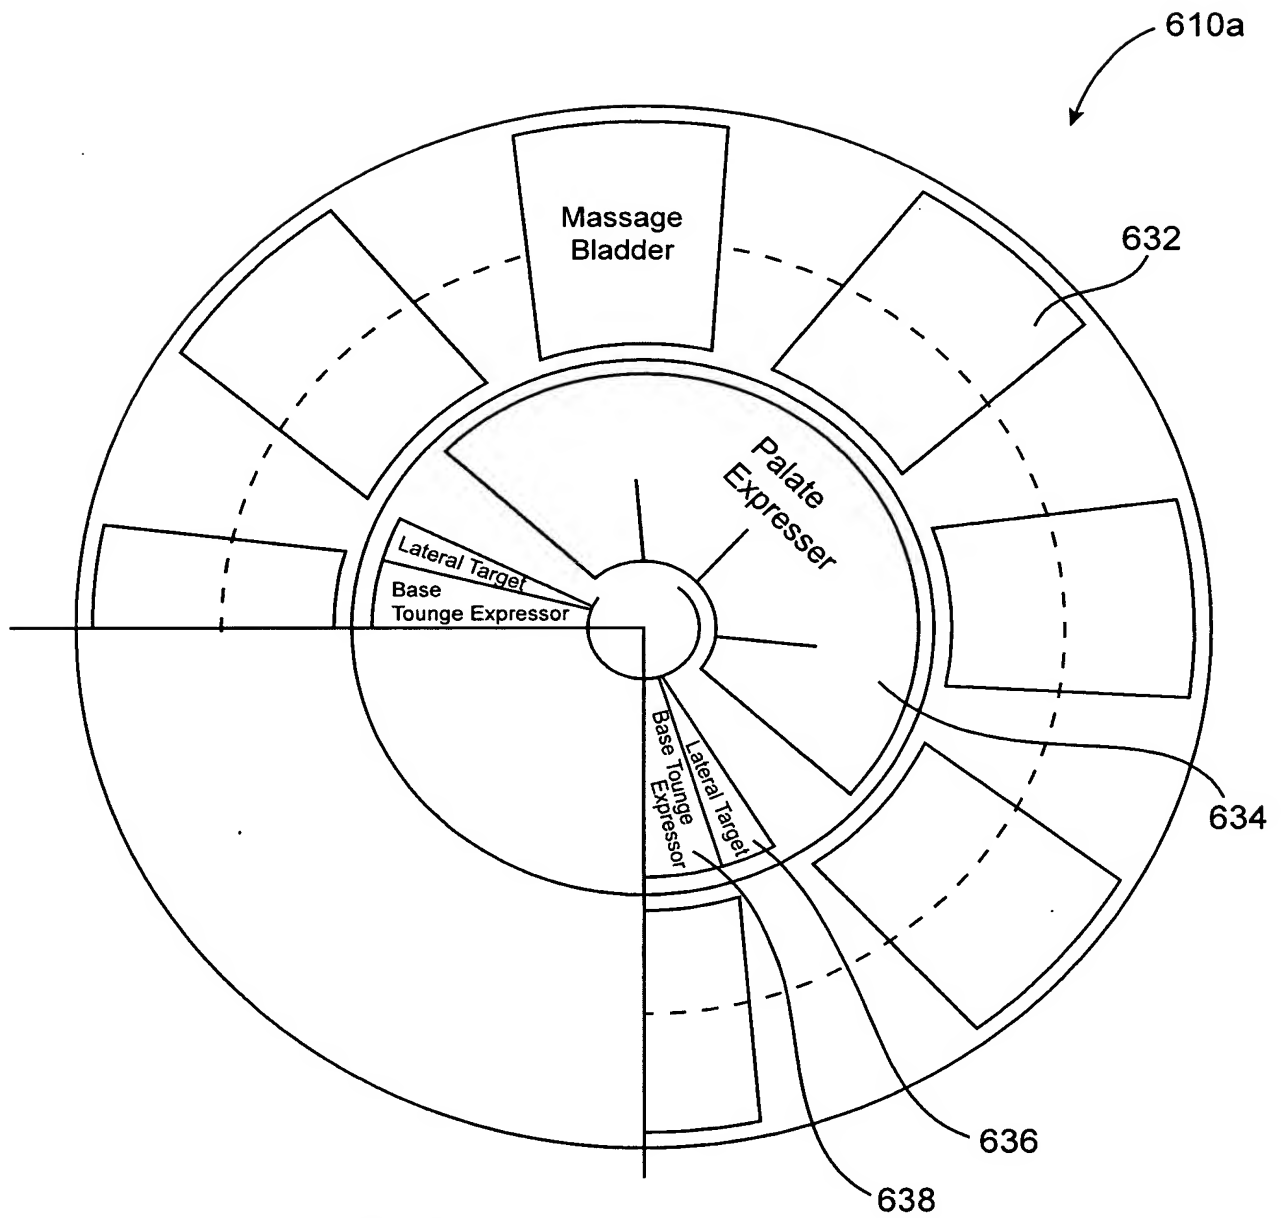


FIG. 8

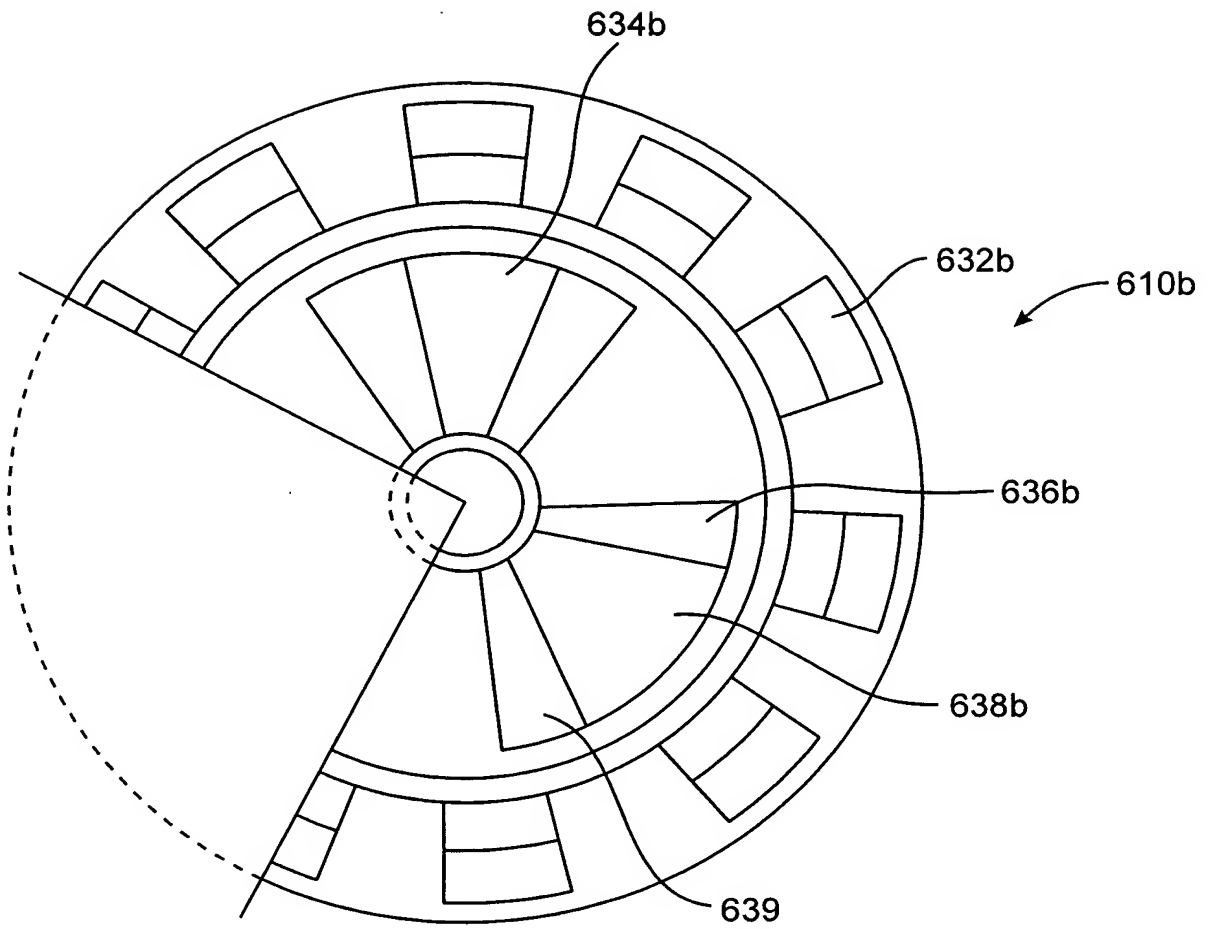


FIG. 9

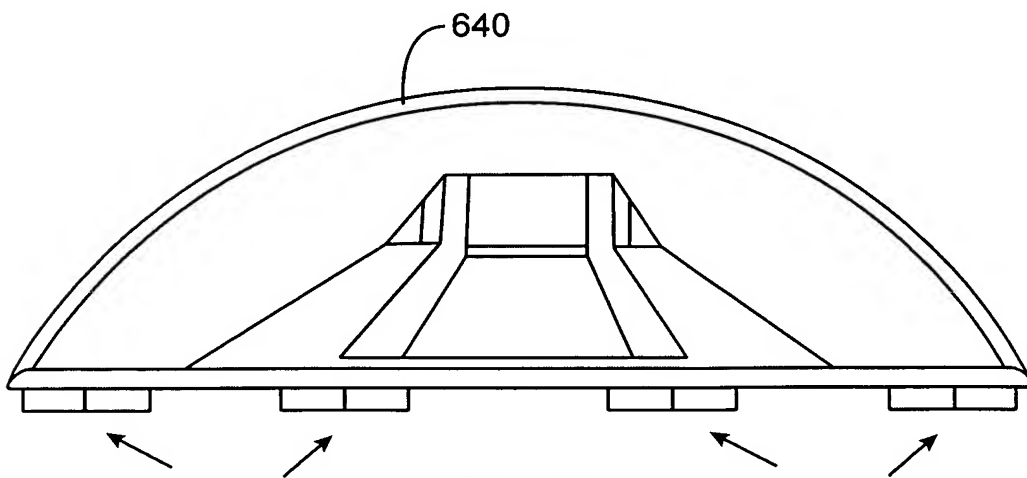


FIG. 10

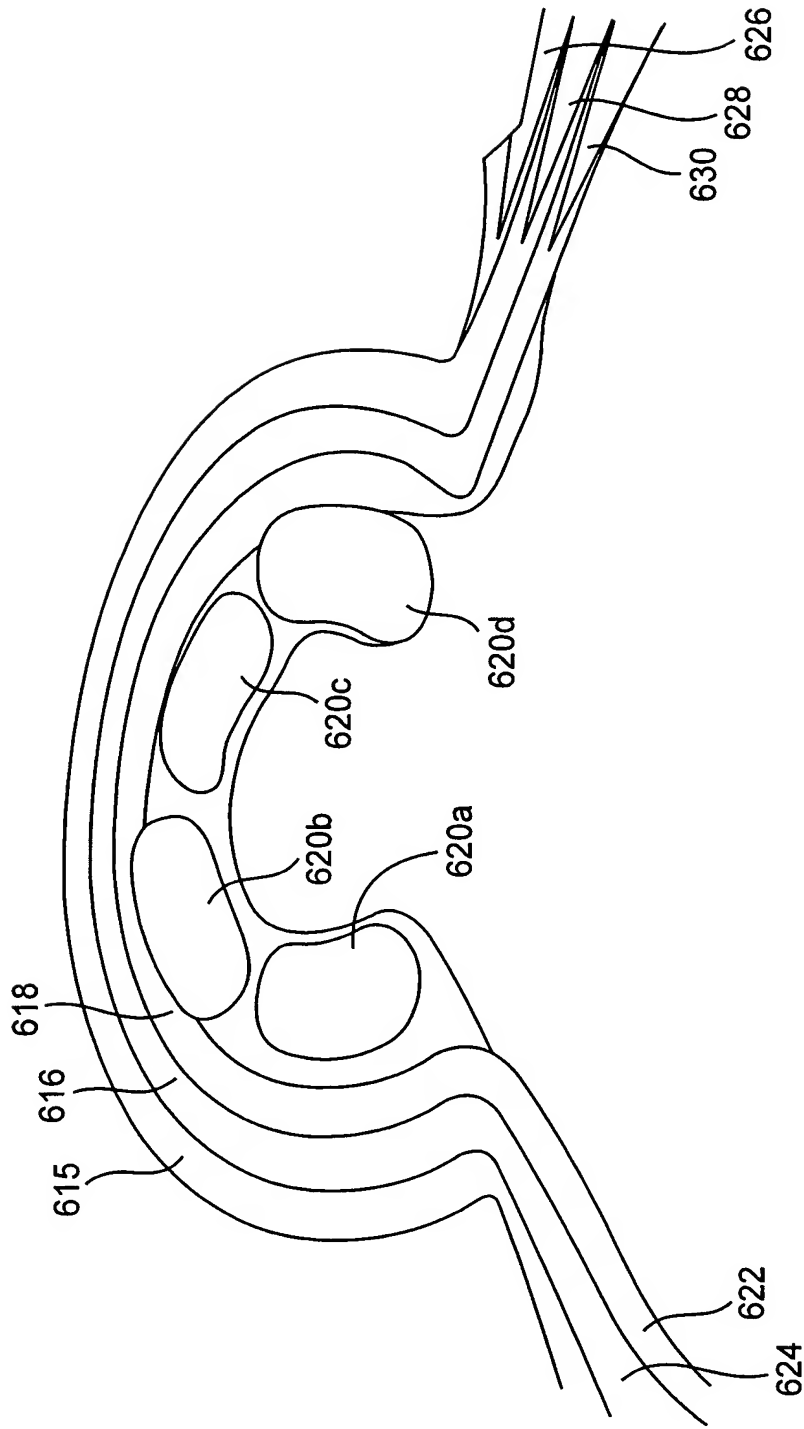


FIG. 11

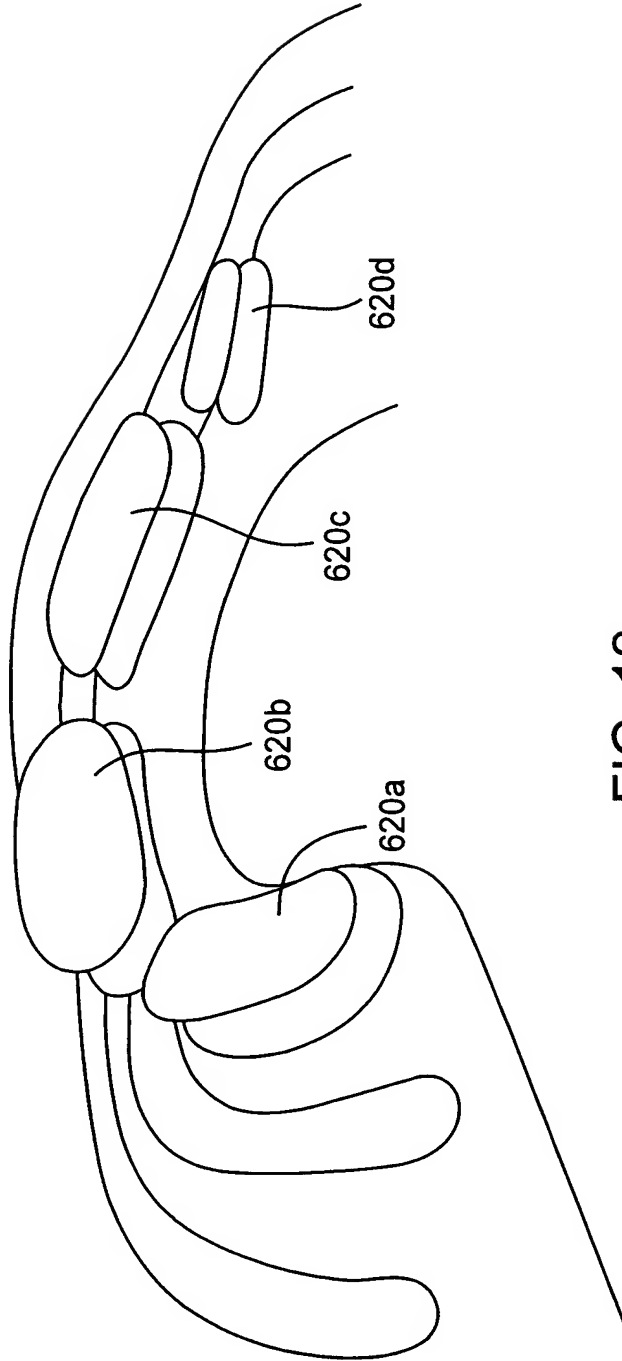


FIG. 12


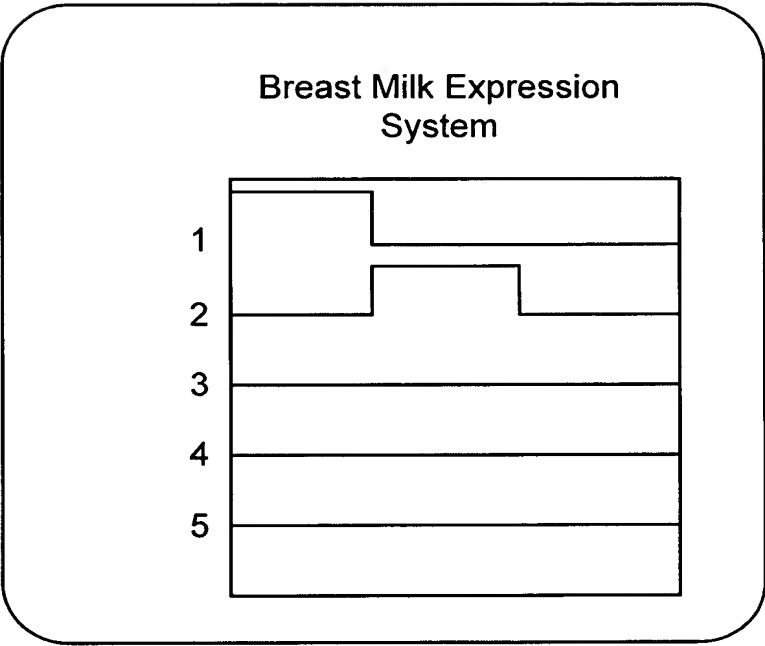


FIG. 13

+

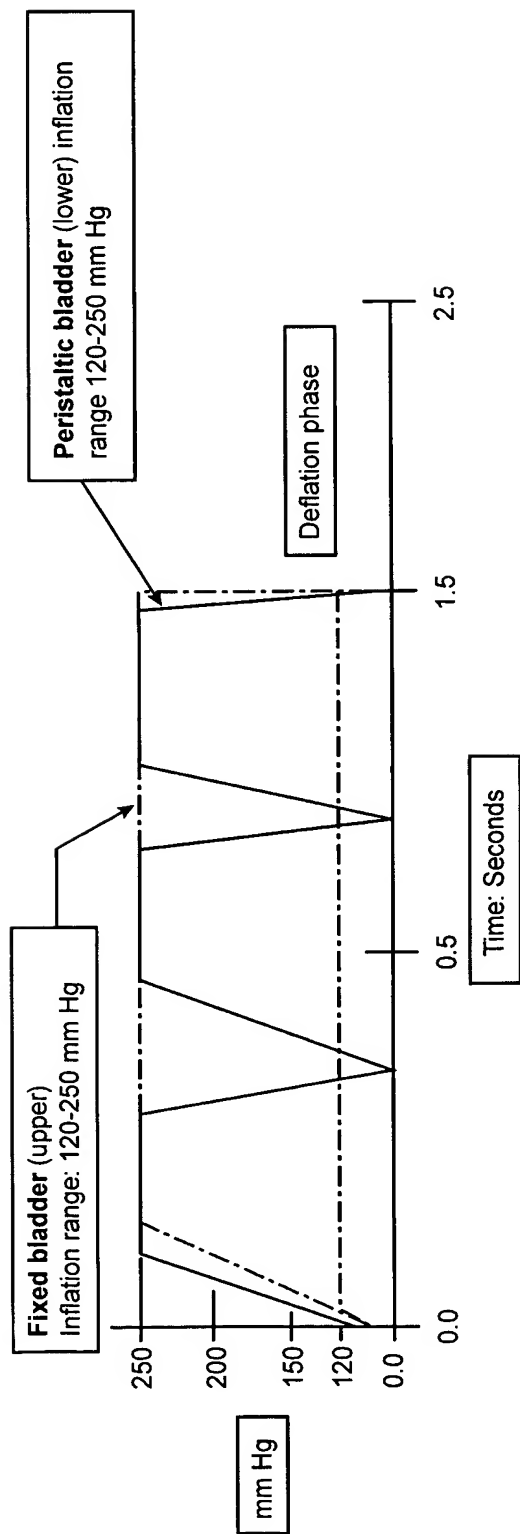

Timing diagram for ring bladder massage system inflation

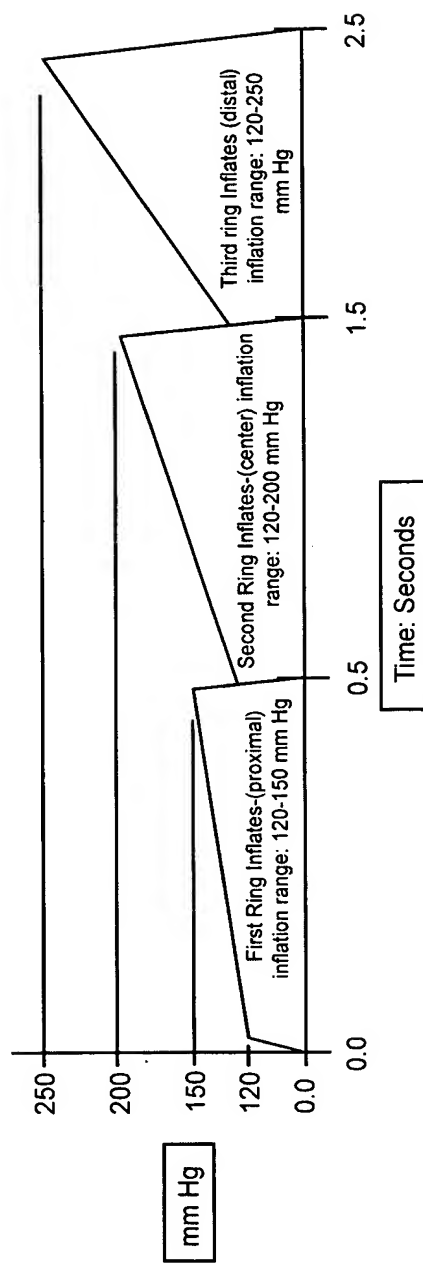


FIG. 14

+

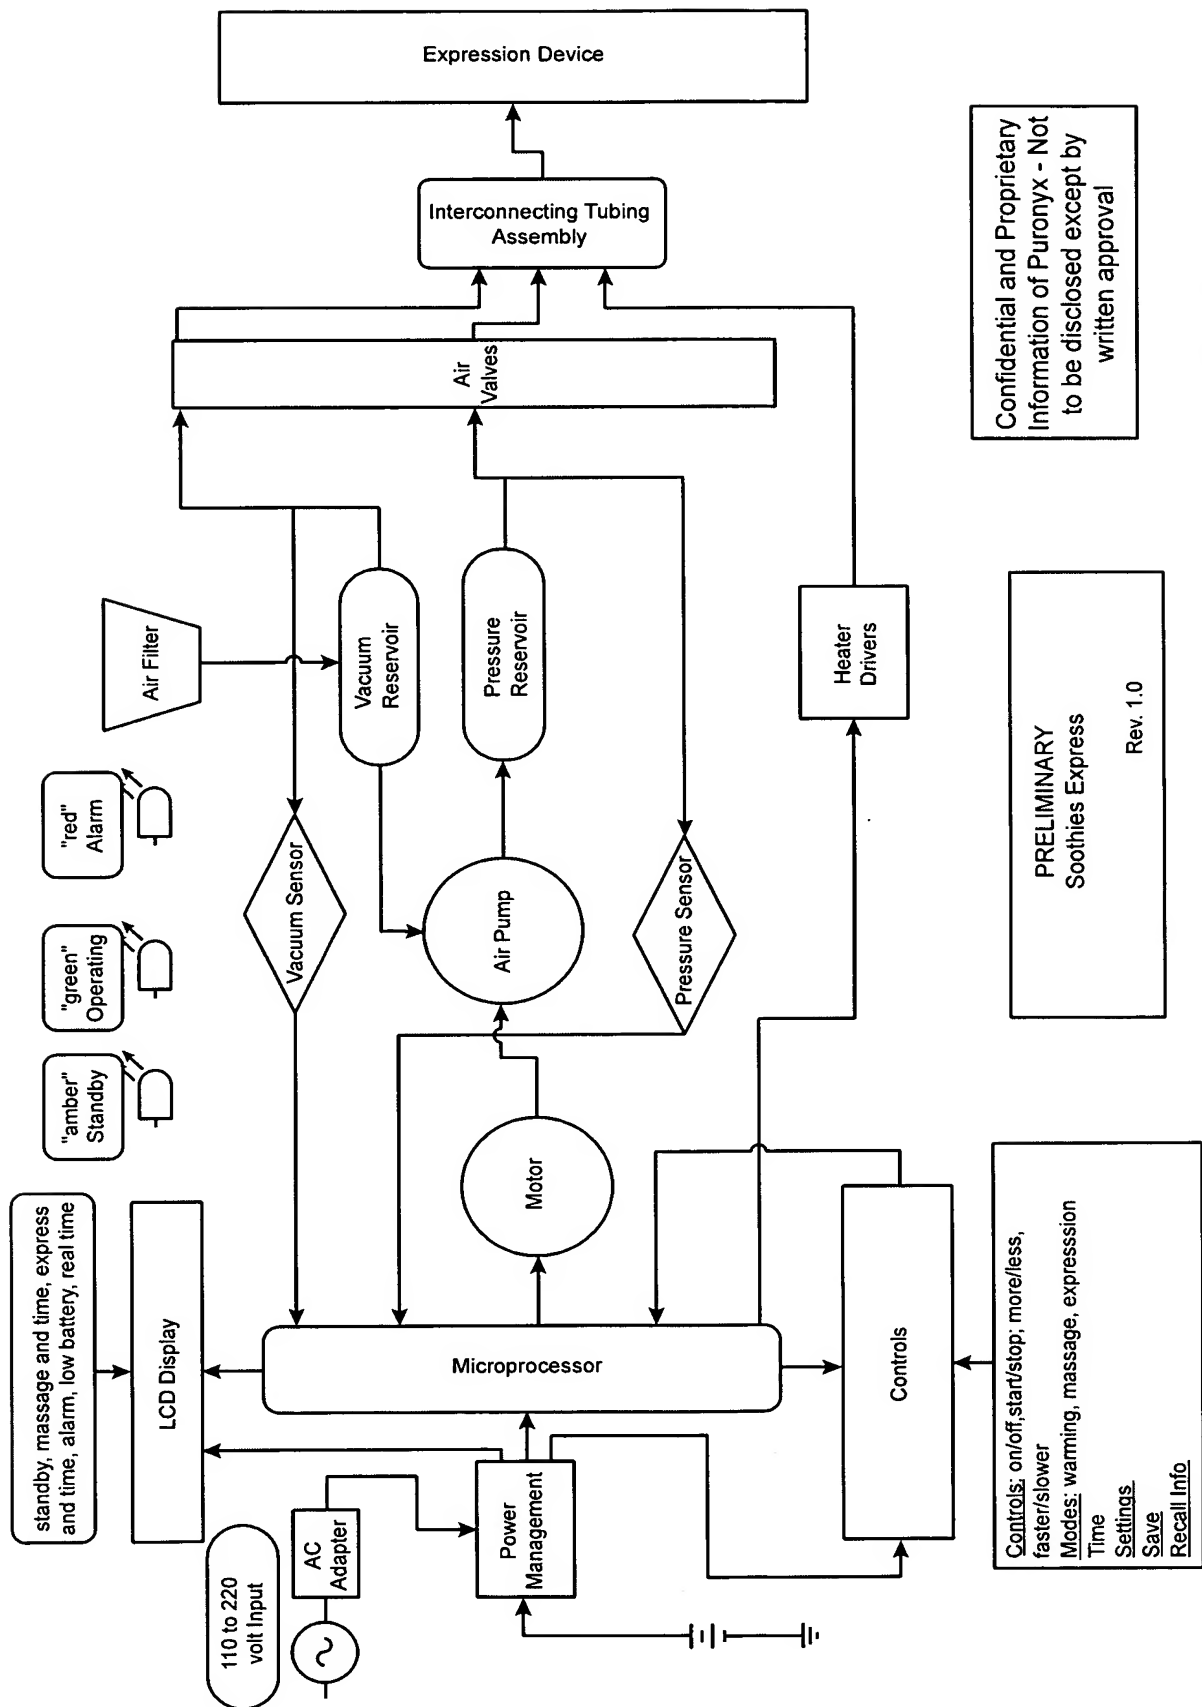


FIG. 15